


TEST REPORT

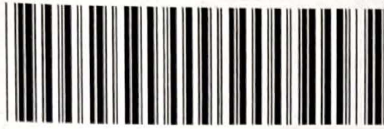

No:200194276

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: UNY0-5620-34

扫码下载报告



ISSUE DATE:2020-07-09

INFORMATION CONFIRMED BY APPLICANT:
4PLY ACTIVATED CARBON DISPOSABLE FACE MASK
QUANTITY: 30 PIECES
MODEL: 34001 175*95mm

DATE RECEIVED/DATE TEST STARTED: 2020-07-02

CONCLUSION:

FORMALDEHYDE CONTENT	M
BACTERIAL FILTRATION EFFICIENCY	M
PARTICLE FILTRATION EFFICIENCY	M
AIRFLOW RESISTANCE	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200194275.
THE DECISION INDICATORS ARE DERIVED FROM THE GROUP STANDARD REQUIRED BY CLIENT (T/CTCA 7-2019).OUR INSPECTION CAPACITY AUTHORIZED BY CMA COVERS THE INSPECTION ITEMS T/CTCA 7-2019.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P.R.CHINA.



APPROVED BY:


Nan Ma ENGINEER

马楠

PAGE 1 OF 3

TEST REPORT

No:200194276

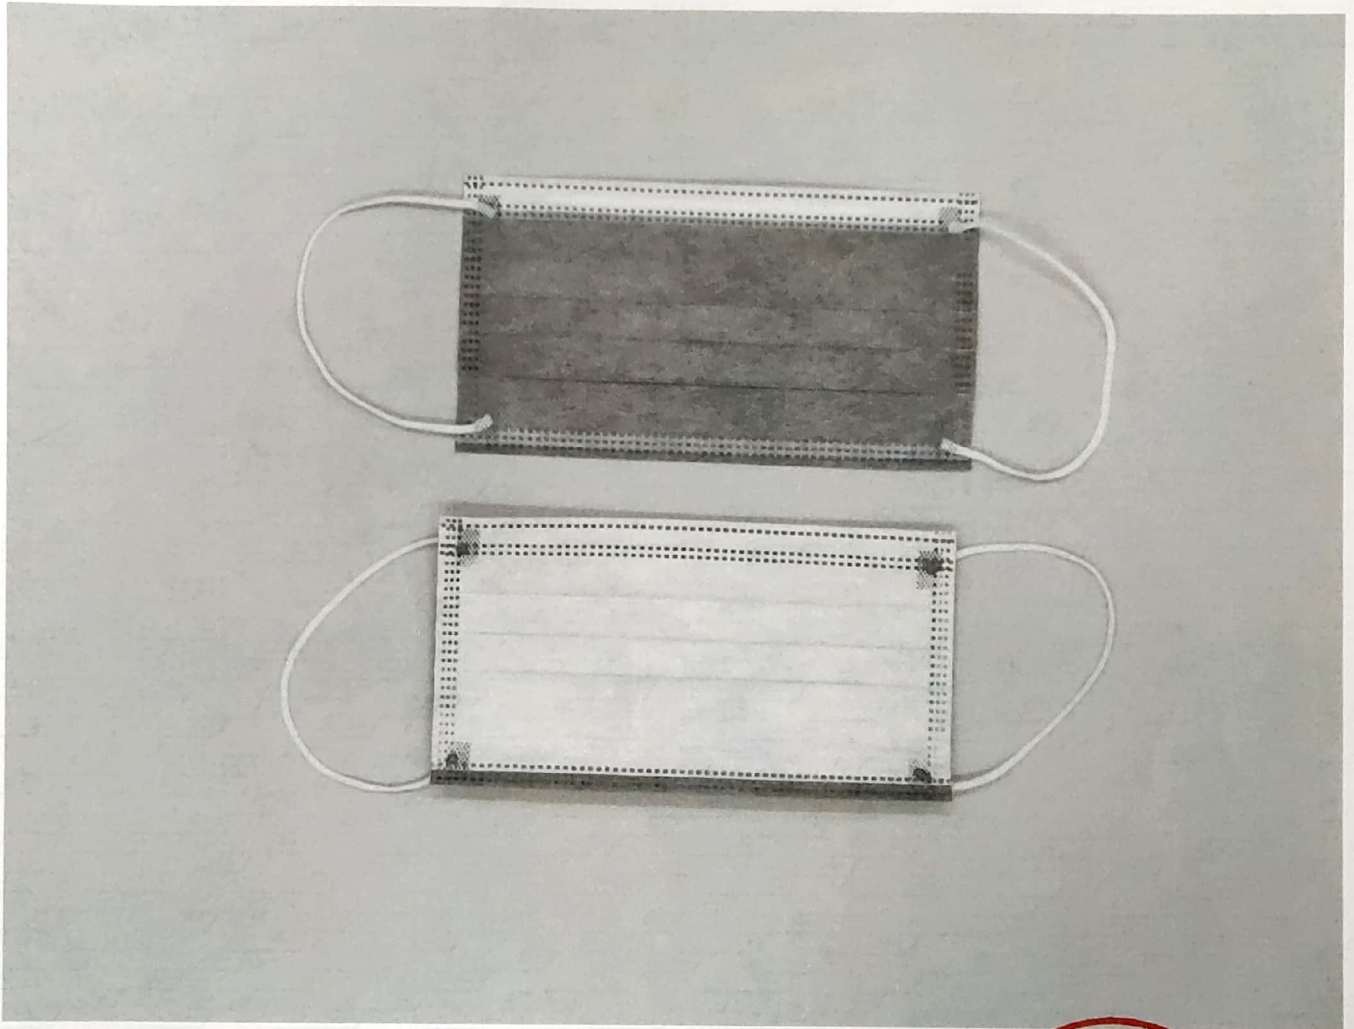

PAGE 2 OF 3

TEST REPORT

No:200194276

FORMALDEHYDE CONTENT

(GB/T 2912.1-2009, WATER EXTRACTION METHOD)
(GB/T 2912.1-2009 mod ISO 14184-1:1998)

NOT DETECTED

REQUIREMENT
 ≤ 20 mg/kg
(T/CTCA 7-2019)

REMARK: DETECTION LIMIT 20mg/kg

BACTERIAL FILTRATION EFFICIENCY (%)

(YY 0469-2011 ANNEX B, TEST BACTERIA: STAPHYLOCOCCUS AUREUS ATCC 6538, TEST AREA:
49cm², FLOW RATE: 28.3L/min, MEAN PARTICLE SIZE: 3.0 μ m, RESULT OF THE POSITIVE
CONTROL: 1.9×10^3 CFU, RESULT OF THE NEGATIVE CONTROL: <1CFU)

BFE₁ 99.6
BFE₂ 99.5
BFE₃ 99.4

REQUIREMENT
 ≥ 95
(T/CTCA 7-2019)

PARTICLE FILTRATION EFFICIENCY (%)

(YY 0469-2011 5.6.2, AIR FLOW: 30L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION:
15mg/m³, TEMP: 23.2°C, RH: 35.1%)

MINIMUM 97.82

REQUIREMENT
 ≥ 80
(T/CTCA 7-2019)

AIRFLOW RESISTANCE (Pa)

(YY 0469-2011 5.6.2, AIR FLOW: 30L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION:
15mg/m³, TEMP: 23.2°C, RH: 35.1%)

MAXIMUM 39.7

REQUIREMENT
 ≤ 80
(T/CTCA 7-2019)



—End of Report—

PAGE 3 OF 3